



! For research use only

Protocol

# Strep-Tactin<sup>®</sup>XT BLI Coupling Kit

## 1 GENERAL INFORMATION & TECHNICAL SPECIFICATIONS

Cat. No.: 2-4380-000

Kit components:

Strep-Tactin <sup>®</sup> XT (53 kDa)	1 mg, lyophilized
EDC	100 mg
s-NHS	57.3 mg
Ethanolamine	20 ml (1 M ethanolamine, pH 8.5)
Immobilization Buffer	30 ml (10 mM sodium acetate, pH 4.5)
10x Buffer W	10 ml (1 M Tris-Cl, 1.5 M NaCl, 10 mM EDTA, pH 8)
Regeneration Buffer	20 ml (3 M GuHCl)

**Required material and reagents:**

- Amine reactive 2G biosensors (AR2G), Cat. No. 18-5092, Sartorius
- 15% w/v Saccharose for preservation of Strep-Tactin<sup>®</sup>XT biosensors

**Storage:**

**Store EDC and lyophilized Strep-Tactin<sup>®</sup>XT at -20 °C.** Store all other kit components at 2-8 °C.

**Stability:**

All products are stable for 6 months after shipping.

**Shipping:**

Cooled with blue ice

**Warnings:**

Warnings are stated on the Material Safety Data Sheet.

**Important information:**

The Strep-Tactin<sup>®</sup>XT BLI Coupling Kit is intended for site-directed, reversible capture of Twin-Strep-tag<sup>®</sup> proteins for biomolecular interaction analysis using Bio-Layer Interferometry (BLI) devices. It is highly recommended to use Twin-Strep-tag<sup>®</sup> instead of Strep-tag<sup>®</sup>II for this approach since the higher affinity of the Twin-Strep-tag<sup>®</sup> to Strep-Tactin<sup>®</sup>XT leads to long-term stable binding on the biosensor surface. The kit components are sufficient for coating of one tray consisting of 96 biosensors. The protocol is adjusted for the Octet<sup>®</sup> instrument and describes coating and measurement with eight biosensors in parallel.

## 2 DESCRIPTION

The Strep-tag® technology is one of the most widely used affinity chromatography systems and it allows, in addition to purification, the detection and immobilization of recombinant proteins. Constant developments of the technology lead to a powerful tool, which is based on the Strep-Tactin®XT in combination with the Twin-Strep-tag® (WSHPQFEK-GGGSGGGSGG-SA-WSHPQFEK), the tandem Strep-tag®II. Strep-Tactin®XT has a binding affinity in low pM range for the Twin-Strep-tag®. This high affinity enables new applications in the field of high-throughput screening and analytic applications like Bio-Layer Interferometry (BLI), making the technology superior to all other available affinity tag systems. The Strep-Tactin®XT BLI Coupling Kit provides all necessary reagents for coating of up to 96 biosensors (one tray) with Strep-Tactin®XT and subsequent capture of Twin-Strep-tag® proteins (ligand) whereby binding affinities and/or kinetics to a specific analyte can be determined. For the measurements, the analyte can be present in culture supernatant, cell extract, or various buffers.

## 3 INITIAL PREPARATIONS

### 3.1 Strep-Tactin®XT stock solution

Dissolve Strep-Tactin®XT in 1 ml of sterile PBS to obtain a 1 mg/ml solution (18.87 µM). Store Strep-Tactin®XT solution at 2-8 °C until needed. The solution is stable for 12 months.

### 3.2 Buffer W working solution

Dilute 1 volume of 10x Buffer W with 9 volumes of water to obtain 1x Buffer W. Store at 2-8 °C until needed.

### 3.3 EDC and s-NHS stock solution

For preparation of stock solutions, it is recommended dissolving each reagent in water and splitting each solution into aliquots of 100 µl. Aliquots of 100 µl will provide enough reagent to perform 8 immobilizations as described in the protocol below.

- 3.3.1** Dissolve EDC in 1300 µl of water to generate a 400 mM stock.
- 3.3.2** Mix to ensure complete dissolution of the solid.
- 3.3.3** Aliquot and freeze immediately at -20 °C. Store there until needed.
- 3.3.4** Dissolve s-NHS in 1320 µl of water to generate a 200 mM stock.
- 3.3.5** Mix to ensure complete dissolution of the solid.
- 3.3.6** Aliquot and freeze immediately at -20 °C. Store there until needed.

Reagent integrity will be maintained for at least 6 months under proper storage conditions. For each experiment, thaw one aliquot of EDC and one of s-NHS. Vortex briefly after thawing. Do not refreeze EDC and s-NHS aliquots. Use EDC and s-NHS within 15 minutes after mixing them together.

## 4 PROTOCOL

### 4.1 Hydration of biosensors



- Hydrate the required number of biosensors in water in a separate hydration plate at room temperature.

- 4.1.1** Pipet 200 µl water per well into a 96-well plate.
- 4.1.2** Insert the hydration plate into the biosensor tray.
- 4.1.3** Align the biosensor rack over the hydration plate and lower the biosensors into the wells, taking care to not scrape or touch the bottom of the biosensors.
- 4.1.4** Hydrate the biosensors for at least 45 minutes at room temperature.

### 4.2 Preparation of Strep-Tactin®XT biosensors for later use




- Equilibrate reagents and samples (except EDC and s-NHS aliquots) to room temperature prior to preparation. For frozen samples, thaw and mix thoroughly prior to use and chill on ice until needed.
- Use EDC and s-NHS within 15 minutes of mixing them together!
- Ensure that the Octet® instrument is turned on and the lamp is warmed up to room temperature for at least 40 minutes prior to starting the assay.

- 4.2.1** Pre-set the assay as indicated in table 1 in the data acquisition software.
- 4.2.2** Prepare a 96-well plate for immobilization and drying as shown in figure 1.
- 4.2.3** Pipet 200 µl/well water into column 1 and 5 of a 96-well plate.
- 4.2.4** Pipet 200 µl/well 1 M Ethanolamine pH 8.5 into column 4.
- 4.2.5** Prepare the required volume of Strep-Tactin®XT working solution. Therefore, dilute Strep-Tactin®XT with immobilization buffer to obtain a concentration of 50 µg/ml. Pipet 200 µl/well Strep-Tactin®XT working solution into column 3.
- 4.2.6** Prepare 2000 µl of an EDC/s-NHS working solution (20 mM EDC, 10 mM s-NHS) by mixing both aliquots and addition 1800 µl of water. Mix thoroughly. Pipet 200 µl/well of the EDC/s-NHS working solution into column 2. Use EDC and s-NHS within 15 minutes of mixing them together!
- 4.2.7** Leave all remaining wells empty.
- 4.2.8** Place both the sample plate and hydration plate with biosensors into the Octet®.
- 4.2.9** Start assay by clicking “GO”.
- 4.2.10** In the case that Strep-Tactin®XT biosensors should be stored for a longer period before being used, it is recommended to preserve them. For preservation of Strep-Tactin®XT biosensors follow the instructions in section “4.4 Preservation of Strep-Tactin®XT biosensors for storage”.

**Table 1: Octet® program for coating of Strep-Tactin®XT biosensors.** \*\* Column refers to the column in the 96-well plate for the immobilization and drying as shown in figure 1.

#	Step	Duration [sec]	Shaker speed [rpm]	Step type	Column**
1	Equilibration	60	1000	Custom	1
2	Activation	300	1000	Activation	2
3	Immobilization	600	1000	Loading	3
4	Quench	300	1000	Quench	4
5	Wash	60	1000	Custom	5

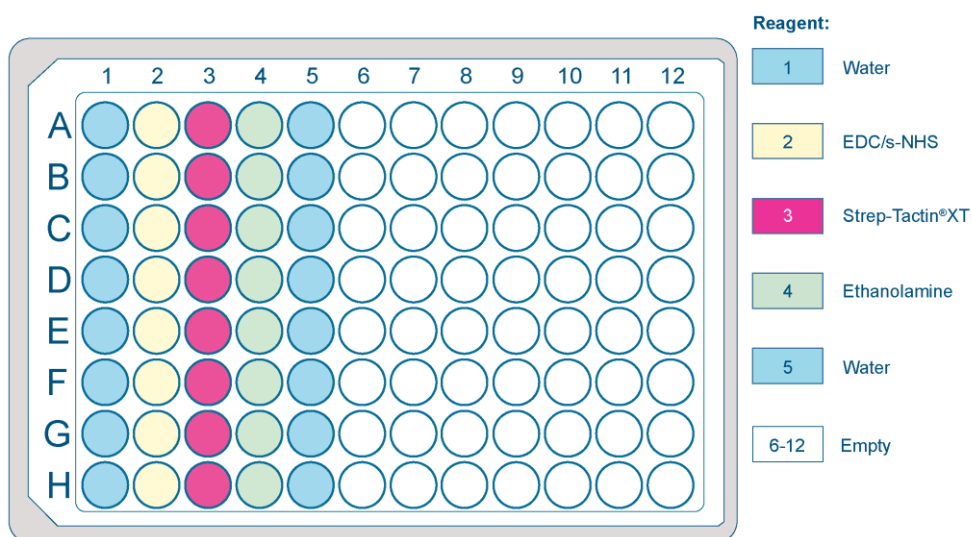

**Figure 1: Pipetting scheme of the 96-well for coating of Strep-Tactin®XT biosensors.** The reagent in each column is color-coded and listed in the legend.

### 4.3 Immobilization of Strep-Tactin®XT to biosensors with subsequent kinetic assay and regeneration




- Equilibrate reagents and samples (except EDC and s-NHS aliquots) to room temperature prior to preparation. For frozen samples, thaw and mix thoroughly prior to use and chill on ice until needed.
- Use EDC and s-NHS within 15 minutes of mixing them together!
- Ensure that the Octet® instrument is turned on and the lamp is warmed up to room temperature for at least 40 minutes prior to starting the assay.
- Instead of 1x Buffer W other buffers can be applied as assay running buffer. Please note that assay running buffer should be used to dilute the Twin-Strep-tag® ligand and the analyte.

- 4.3.1** Pre-set the assay as indicated in table 2 in the data acquisition software.
- 4.3.2** Prepare a 96-well plate for immobilization, assay and regeneration as shown in figure 2.
- 4.3.3** Pipet 200 µl/well water into column 1 and 11.
- 4.3.4** Pipet 200 µl/well 1 M ethanolamine pH 8.5 into column 4.
- 4.3.5** Pipet 200 µl/well 1x Buffer W or your desired assay running buffer into column 5, 7 and 9.
- 4.3.6** Pipet 200 µl/well Regeneration Buffer into column 10.
- 4.3.7** Prepare the Twin-Strep-tag® ligand in assay running buffer and pipet 200 µl/well of the Twin-Strep-tag® ligand into column 6.
- 4.3.8** Prepare analyte in assay running buffer and pipet 200 µl/well of the analyte into column 8.
- 4.3.9** Prepare the required volume of Strep-Tactin®XT working solution. Therefore, dilute Strep-Tactin®XT with immobilization buffer to obtain a concentration of 50 µg/ml. Pipet 200 µl/well of Strep-Tactin®XT into column 3.

- 4.3.10** Prepare 2000 µl of an EDC/s-NHS working solution (20 mM EDC, 10 mM s-NHS) by mixing both aliquots and addition 1800 µl of water. Mix thoroughly. Pipet 200 µl/well of the EDC/s-NHS working solution into column 2. Use EDC and s-NHS within 15 minutes of mixing them together!
- 4.3.11** Leave all remaining wells empty.
- 4.3.12** Place both the sample plate and hydration plate with biosensors into the Octet®.
- 4.3.13** Start assay by clicking “GO”.
- 4.3.14** In the case that Strep-Tactin®XT biosensors should be stored for a longer period before being reused, it is recommended to preserve them. For preservation of Strep-Tactin®XT biosensors follow the instructions in section “4.4 Preservation of Strep-Tactin®XT biosensors for storage”.

**Table 2: Octet® program for coating of Strep-Tactin®XT biosensors, subsequent kinetic assay, and regeneration.** \* Duration of binding of the Twin-Strep-tag® ligand (#6), binding of the analyte (#8) and dissociation of the analyte (#9) depend on the specifications of ligand and analyte and have to be determined experimentally. \*\* Column refers to the column in the 96-well plate for the immobilization, assay and regeneration as shown in figure 2.

#	Step	Duration [sec]	Shaker speed [rpm]	Step type	Column**
1	Equilibration	60	1000	Custom	1
2	Activation	300	1000	Activation	2
3	Immobilization	600	1000	Loading	3
4	Quench	300	1000	Quench	4
5	Initial baseline	60	1000	Initial baseline	5
6	Binding of Twin-Strep-tag® ligand	custom*	1000	Loading	6
7	Baseline	60	1000	Baseline	7
8	Binding of analyte	custom*	1000	Association	8
9	Dissociation of analyte	custom*	1000	Dissociation	9
10	Regeneration	60	1000	Custom	10
11	Wash	60	1000	Custom	11

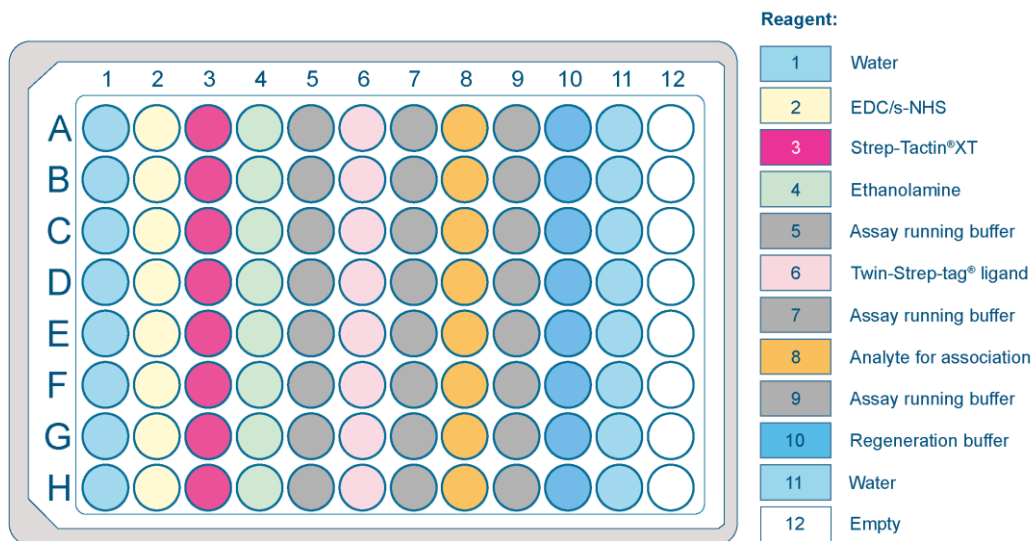

**Figure 2: Pipetting scheme of the 96-well plate for coating of Strep-Tactin®XT biosensors, subsequent kinetic assay, and regeneration.** The reagent in each column is color-coded and listed in the legend.

#### 4.4 Preservation of Strep-Tactin®XT biosensors for storage



- Preservation of the Strep-Tactin®XT biosensors occur offline in the biosensor tray holder.

- 4.4.1** Determine the number of biosensors to be preserved for storage.
- 4.4.2** Prepare a separate 96-well plate and fill the wells that match the location of the biosensors with 15% w/v Saccharose (200 µl/well).
- 4.4.3** Insert the preservation plate into the biosensor tray.
- 4.4.4** Align the biosensor rack over the hydration plate and lower the biosensors into the wells, taking care to not scrape or touch the bottom of the biosensors.
- 4.4.5** Incubate the biosensors for 2 minutes at room temperature.
- 4.4.6** Transfer Strep-Tactin®XT coated biosensors into an empty biosensor tray and let them dry at room temperature for 5 minutes.
- 4.4.7** Keep the Strep-Tactin®XT biosensors dry and dark at room temperature until use. Before next use, hydrate the Strep-Tactin®XT biosensors for at least 10 minutes in assay running buffer.

# End User Limited Use License

By and between  
**IBA Lifesciences GmbH**  
Göttingen  
("SELLER")

and  
**Purchaser of**  
Licensed Protein (as defined below)  
("PURCHASER")

NOTICE: PURCHASE OF THIS PRODUCT IS ALSO SUBJECT TO IBA GmbH TERMS AND CONDITIONS OF SALE. A COMPLETE COPY OF SUCH TERMS AND CONDITIONS ARE FOUND AT <https://www.iba-lifesciences.com/terms-and-conditions.html>

IN THE EVENT THAT ANY TERMS OR CONDITIONS OF THIS END USER LIMITED USE LICENSE (the "LIMITED USE LICENSE") AND IBA GmbH's TERMS AND CONDITIONS OF SALE CONFLICT OR IN CASE OF ANY DOUBT, THE MOST RESTRICTIVE TERMS AND CONDITIONS SHALL APPLY TOWARDS THE PURCHASER.

The compound(s) you have purchased (the "Licensed Protein", as specifically defined below), and/or the use thereof, may be covered by claims in the following patents controlled by IBA GmbH (collectively "Patent Rights"):

## PATENT RIGHTS

A) SEQUENTIALLY ARRANGED STREPTAVIDIN-BINDING MODULES AS AFFINITY TAGS  
US Patent No. 7,981,632  
US Patent No. 8,735,540  
DE Patent No. 101 13 776  
EP Patent No. 1370574

B) STREPTAVIDIN MUTEINS AND METHODS OF USING THEM  
US Patent No. 10,065,996  
US Patent No. 11,168,116  
EP Patent No. 2 920 204  
CN Patent No. 3481362  
AU Patent No. 2017257203  
JP Patent No. 6475630

## 1. Definitions.

Whenever used in this Limited Use License document with an initial capital letter, the terms defined below, whether used in the singular or the plural, shall have the meanings specified below.

**1.1 "Commercial Purpose"** means any activity conducted in exchange for consideration including, but not limited to, (a) use of the Tag in research and development activities of a commercial entity or in manufacturing, (b) use of the Tag to provide a service, information or data, other than to perform Contract Research (as defined below), (c) use of the Tag for therapeutic, diagnostic or prophylactic purposes and (d) sale of the Tag, whether or not such Tag is resold for use in research. As used herein, "Contract Research" means Bio-Layer Interferometry (BLI) analysis services performed by a company on a fee-for-service basis wherein said company receives the Tag from their customers and wherein said company uses said Tag within Bio-Layer Interferometry (BLI) analysis only.

**1.2 "Licensed Protein"** shall mean Strep-Tactin XT as described in and protected by the Patent Rights (B), the use of which but for this Limited Use License would infringe one or more Valid Claims of Patent Rights (B).

**1.3 "Tag"** shall mean a protein or any other molecule comprising the amino acid sequence SAWSHQPQFEKGGGGGGSSAWSHQPQFEK described in and protected by the Patent Rights (A), the use of which but for this Limited Use License would infringe one or more Valid Claims of Patent Rights (A).

**1.4 "Field"** shall mean immobilization of Licensed Protein on a solid support (e.g. a biosensor) that is dedicated to enable Bio-Layer Interferometry (BLI) and using said solid support for the binding of molecules comprising the Tag.

**1.5 "Valid Claim"** means: (a) a claim of an issued and unexpired patent within the Patent Rights that has not been (i) held permanently revoked, unenforceable, unpatentable or invalid by a decision of a court or governmental body of competent jurisdiction, unappealable or unappealed within the time allowed for appeal, (ii) rendered unenforceable through disclaimer or otherwise, (iii) abandoned, or (iv) lost through an interference proceeding; or (b) a pending claim of a pending patent application within the Patent Rights that (i) has been asserted and continues to be prosecuted in good faith and (ii) has not been abandoned or finally rejected without the possibility of appeal or refiling.

## 2. Limited Use License.

This Limited Use License assumes and is valid only if you acquired Licensed Protein from IBA. By purchasing Licensed Protein, you explicitly agree with the terms and conditions of this Limited Use License.

This Limited Use License grants to the Purchaser the non-transferable right to use the amount of Licensed Protein purchased by the Purchaser limited to the Field. By purchasing Licensed Protein, Purchaser agrees that (a) Purchaser shall not sell or otherwise transfer Licensed Protein to any other party, (b) Purchaser shall not use the amount of Licensed Protein purchased by such Purchaser beyond the Field, (c) Purchaser shall use Licensed Protein for Commercial Purposes only after having also received an appropriate license for the Tag from Seller (whereas, for sake of clarity, Seller in its own discretion may decide, in particular, (i) whether to grant such license to Purchaser or not, (ii) on the terms and conditions of such license as well as (iii) with respect to any consideration for such license grant), (d) Purchaser shall use Licensed Protein as well as the Tag in compliance with all applicable license terms and conditions, laws and regulations, including, without limitation, applicable human health and animal welfare laws and regulations, (e) Purchaser may transfer information or materials made through the use of Licensed Protein and Tag to a scientific collaborator only if such transfer is not for Commercial Purposes, and that such collaborator agrees in writing not to transfer such materials to any third party and to use such transferred materials and/or information solely for internal, non-clinical research and not for Commercial Purposes and (f) Licensed Protein and Tag have not been approved for use in humans by the U.S. Food and Drug Administration or any other regulatory body and may not be used in humans.

## 3. WARRANTY AND LIABILITY.

EXCEPT FOR FRAUDULENT INTENT (*ARGLIST*), AND/OR WHERE WE HAVE EXPLICITLY ACCEPTED A GUARANTEE FOR THEIR STATE, (*BESCHAFFENHEITSGARANTIE*), THE LICENSED PROTEIN AND THE PATENT RIGHTS ARE PROVIDED AS-IS AND WITH NO WARRANTY, EITHER EXPRESS OR IMPLIED, AND SPECIFICALLY WITHOUT ANY WARRANTY OF MERCHANTABILITY, NON-INFRINGEMENT OR FITNESS FOR A PARTICULAR PURPOSE. EXCEPT FOR LIABILITY FOR INTENTION (*VORSATZ*) AND TO THE EXTENT OTHERWISE PERMITTED BY LAW, UNDER NO CIRCUMSTANCES SHALL SELLER BE LIABLE FOR ANY CLAIMS, DEMANDS, LIABILITIES, COSTS, LOSSES, DAMAGES OR EXPENSES (INCLUDING LEGAL COSTS AND ATTORNEY'S FEES) OF WHATEVER KIND OR NATURE CAUSED TO OR SUFFERED BY ANY PERSON OR ENTITY THAT DIRECTLY OR INDIRECTLY ARISE OUT OF OR RESULT FROM OR ARE ENCOUNTERED IN CONNECTION WITH THE USE OF THE LICENSED PROTEIN OR IN THE FIELD. PURCHASER SHALL INDEMNIFY AND HOLD SELLER HARMLESS FROM AND AGAINST ANY AND ALL CLAIMS, DAMAGES, COSTS, EXPENSES AND OTHER LIABILITIES WITH RESPECT TO THE LICENSED PRODUCTS, FIELD AND THE PATENT RIGHTS.

## 4. Applicable Laws and Legal Venue.

This Label License is subject to and governed by the laws of Germany excluding the international conflict of law provisions. Exclusive legal venue shall be the courts being competent for the business seat of the Seller.



Check our Downloads page

<https://www.iba-lifesciences.com/downloadcenter/>

for the latest version of this manual.



Info on warranty / licensing and trademarks available at:

<https://www.iba-lifesciences.com/patents-licenses-trademarks/>



If you have any questions, please contact

[strep-tag@iba-lifesciences.com](mailto:strep-tag@iba-lifesciences.com)

We are here to help!

